

1

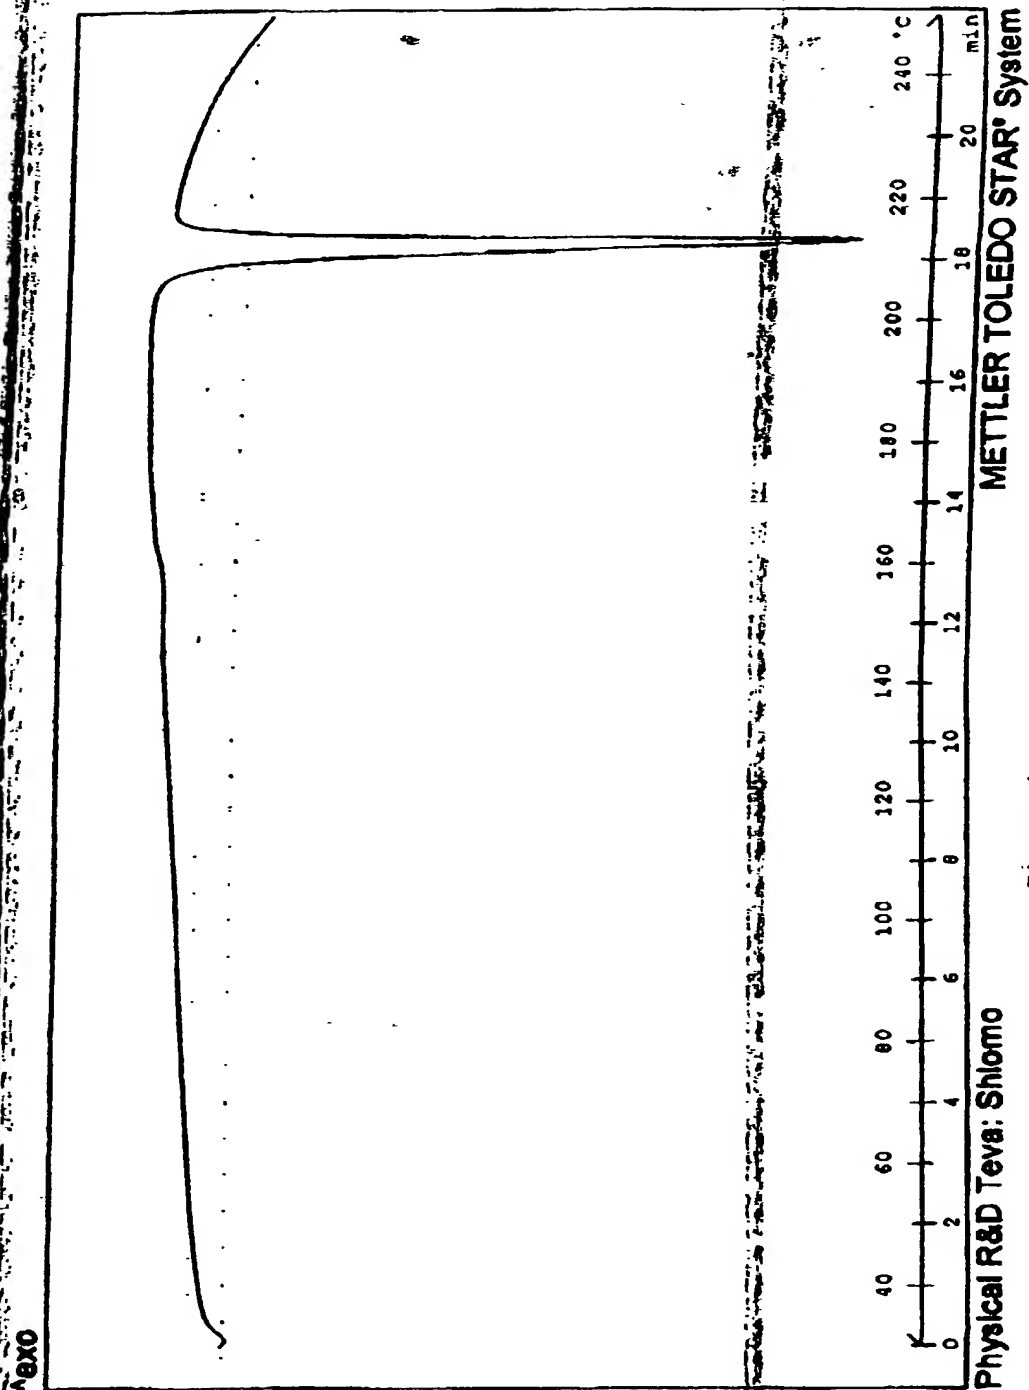


Figure 1




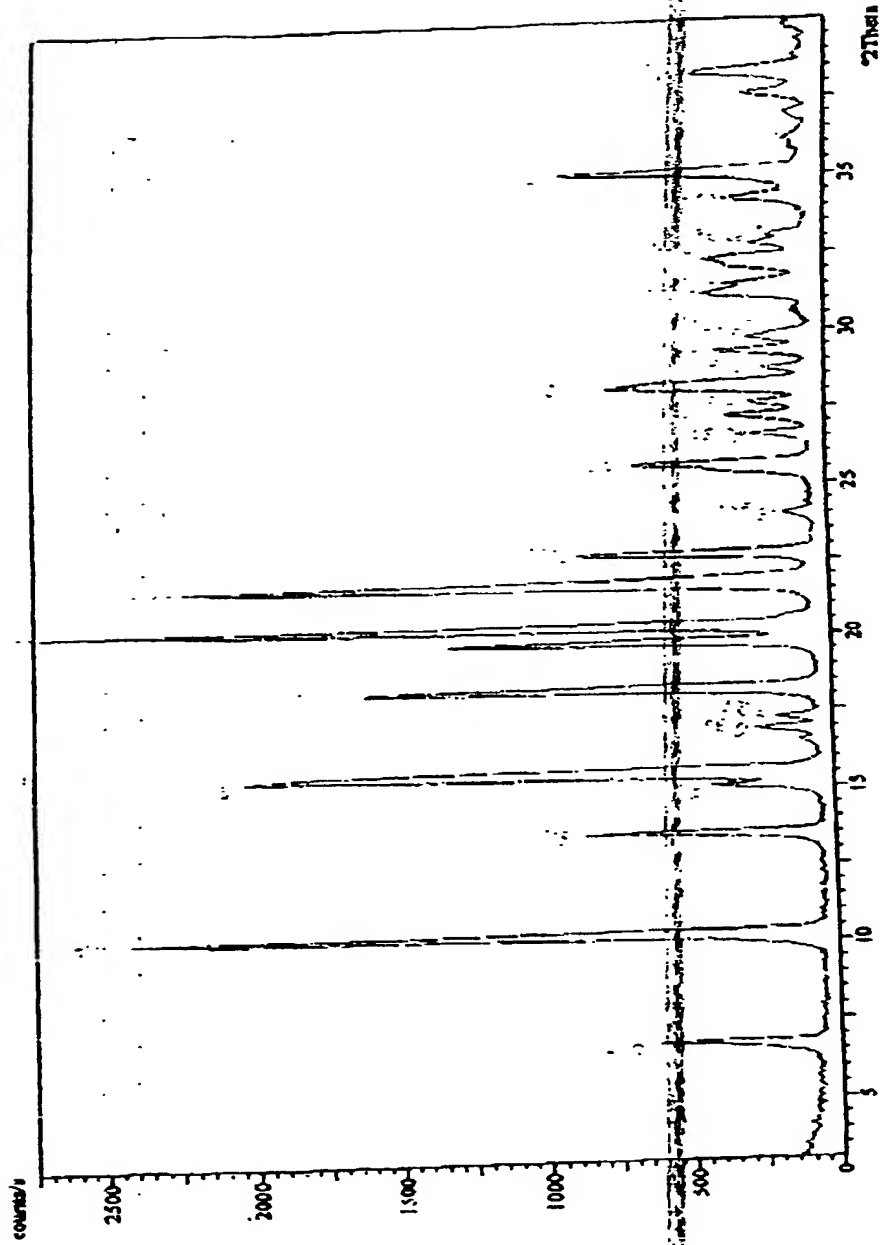


Figure 2



II

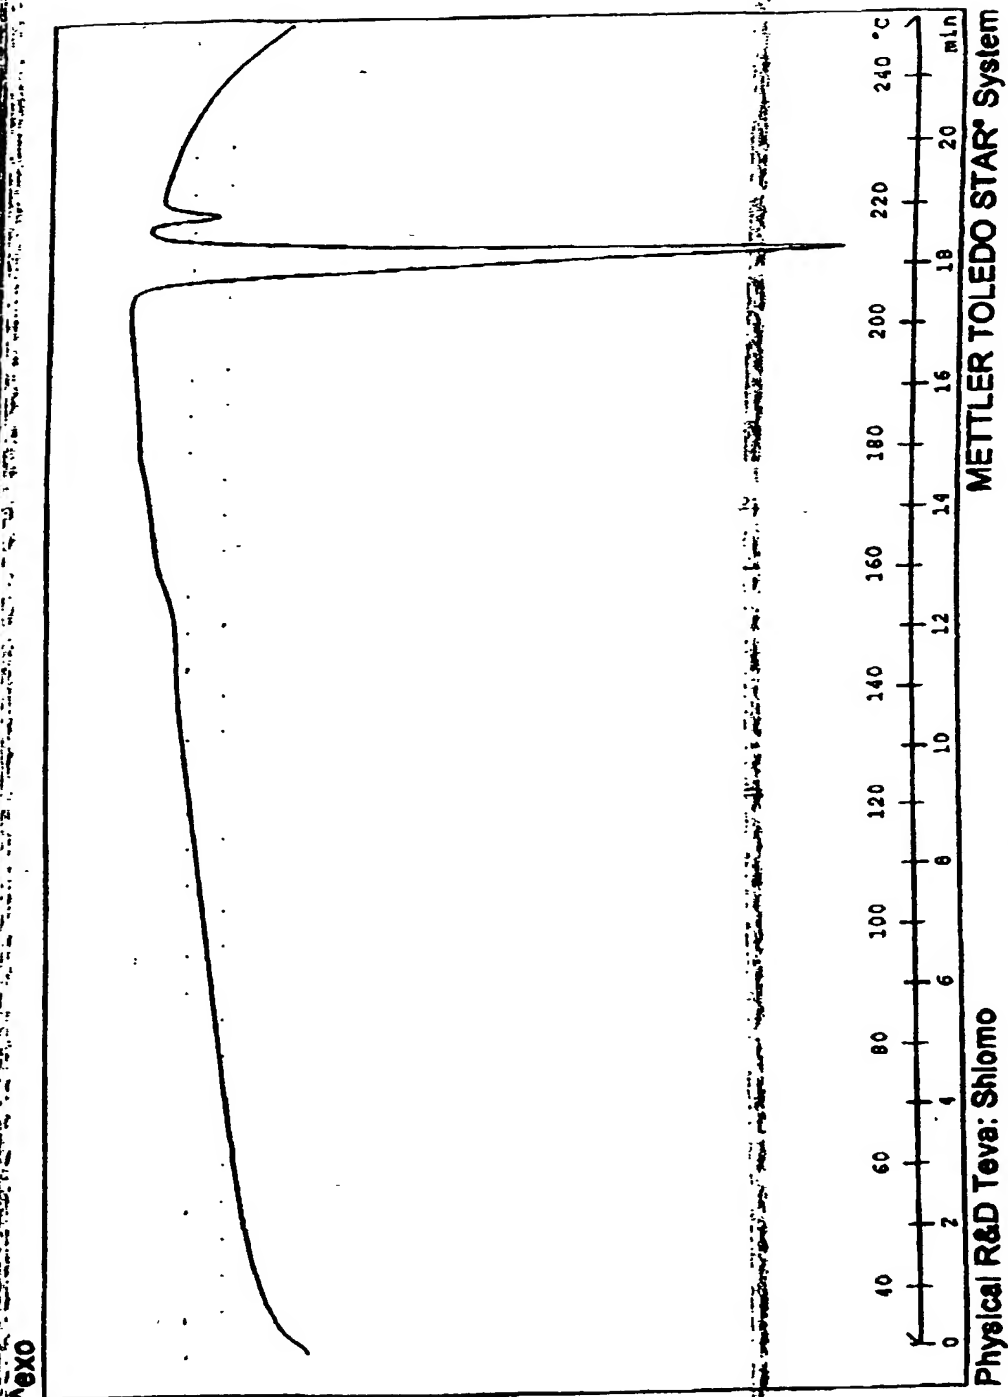


Figure 3



II


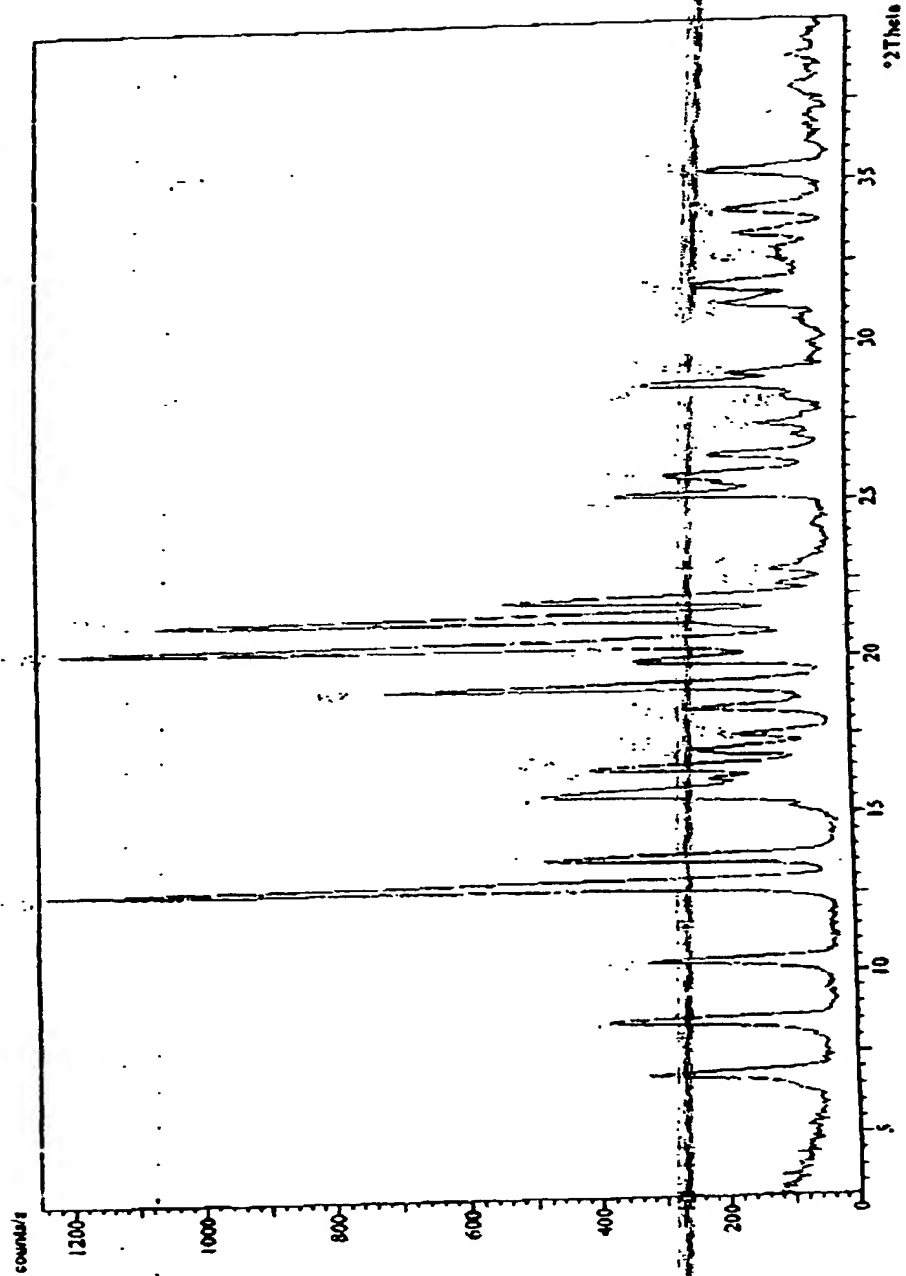


Figure 4



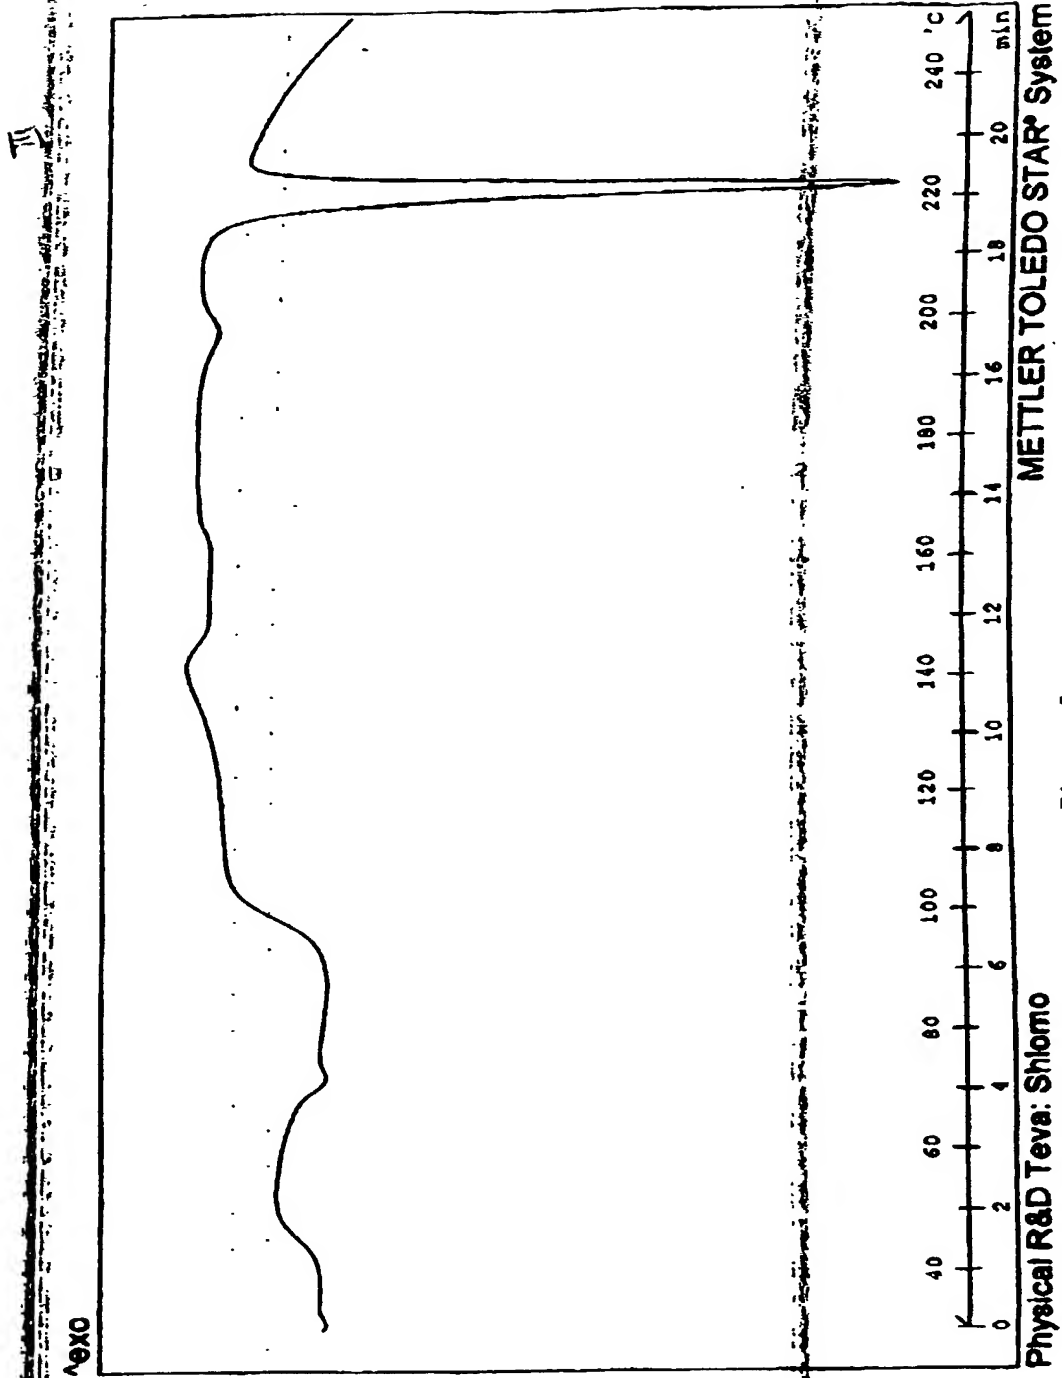

TOTAL P. 03

III


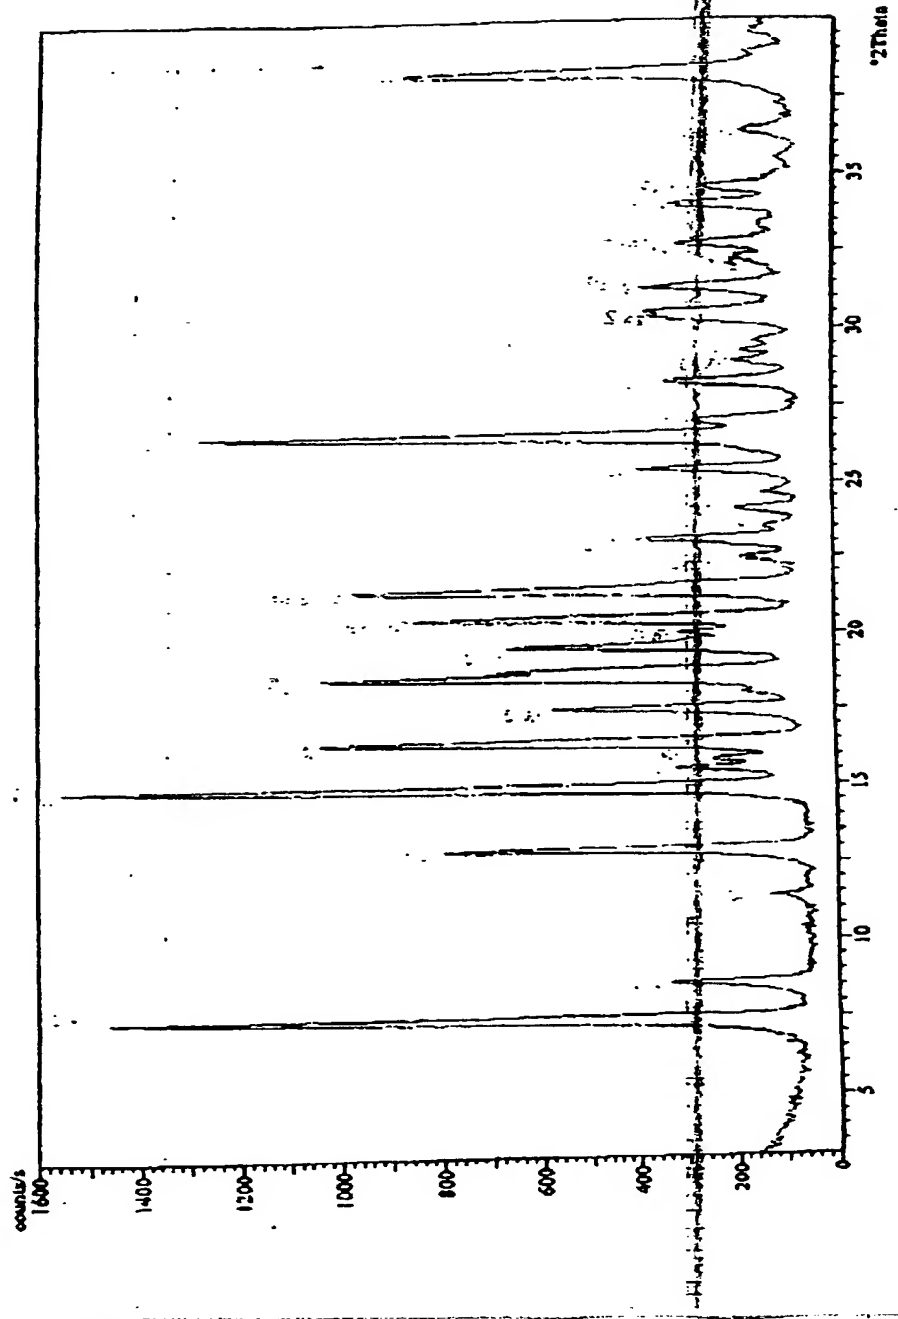


Figure 6

TV

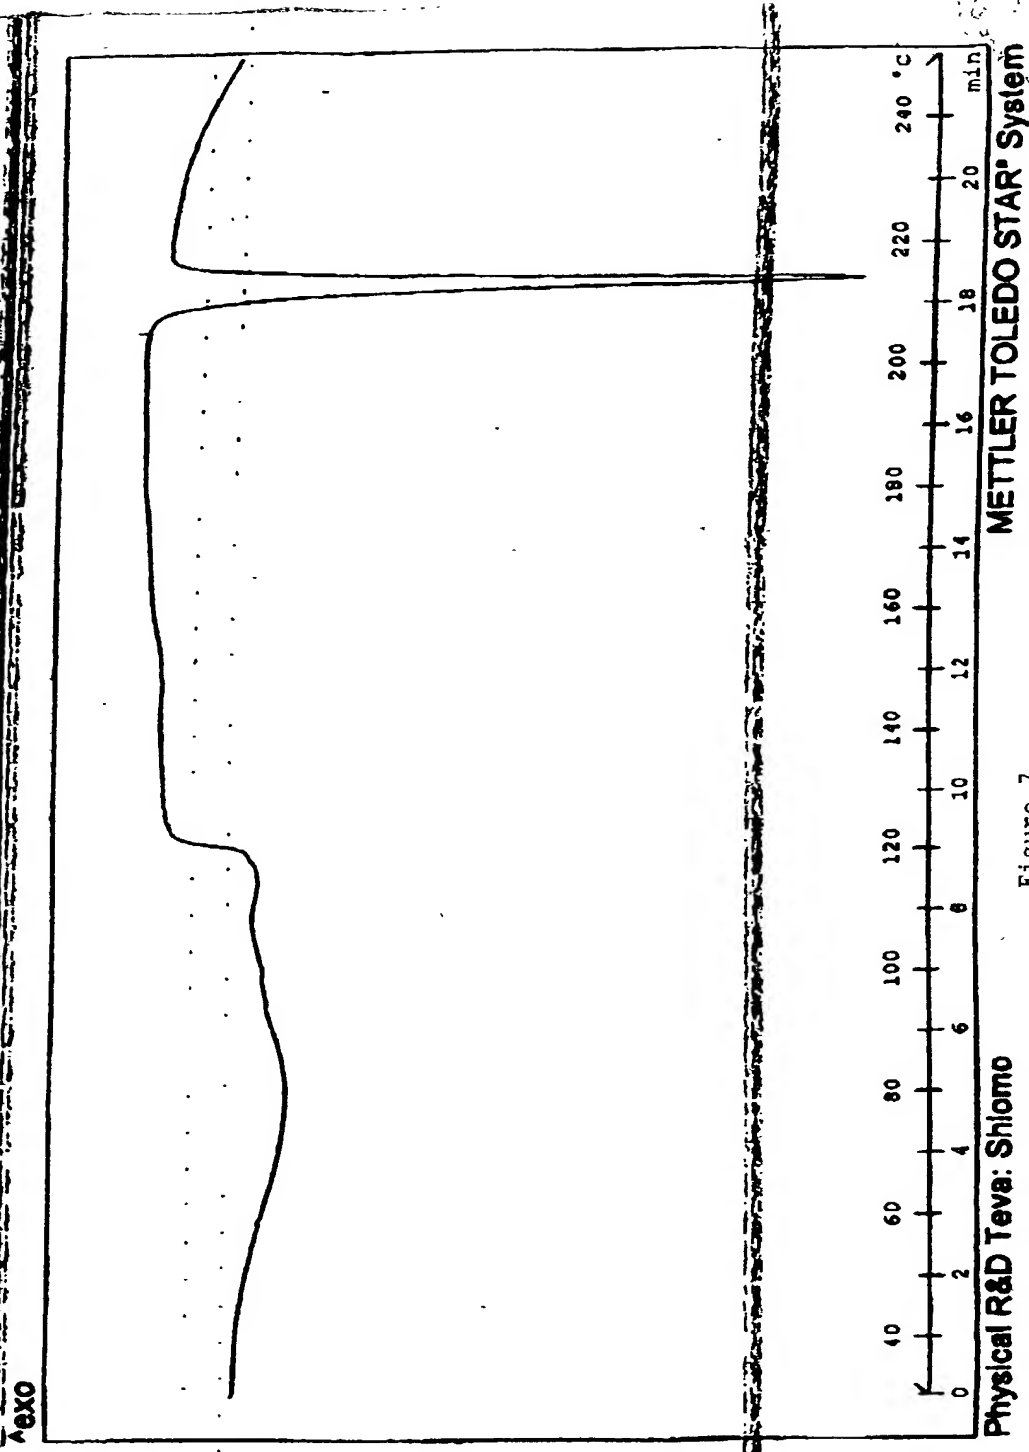

Physical R&D Teva: Shlomo

Figure 7



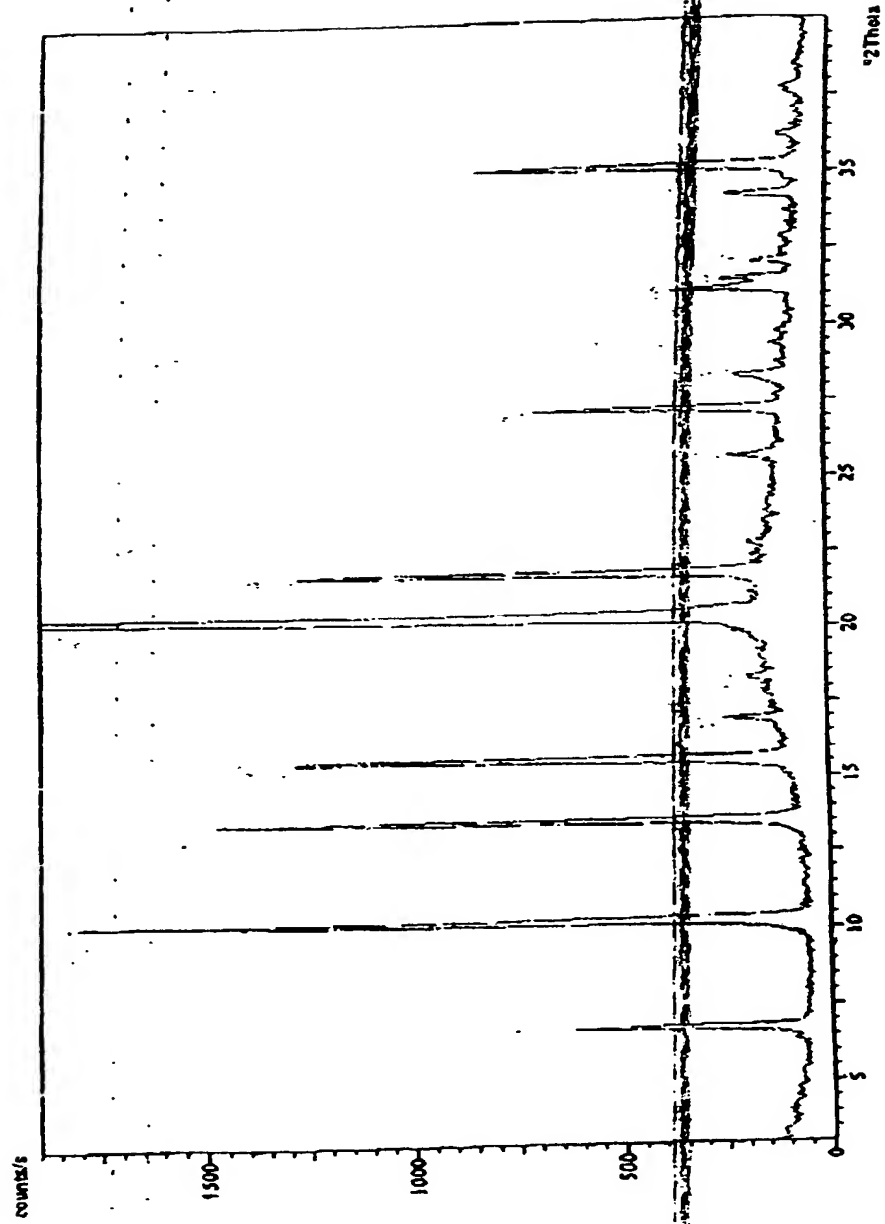


Figure 8



File: VML-07 SHQ, ID: VML-07 SHQ.  
 Date: 02/01/01 15:16 Step: 0.050° Cnt Time: 1.000 Sec.  
 Range: 2.00 - 40.00 (Deg) Cent. Scan Rate: 3.00 Deg/min. TSVX

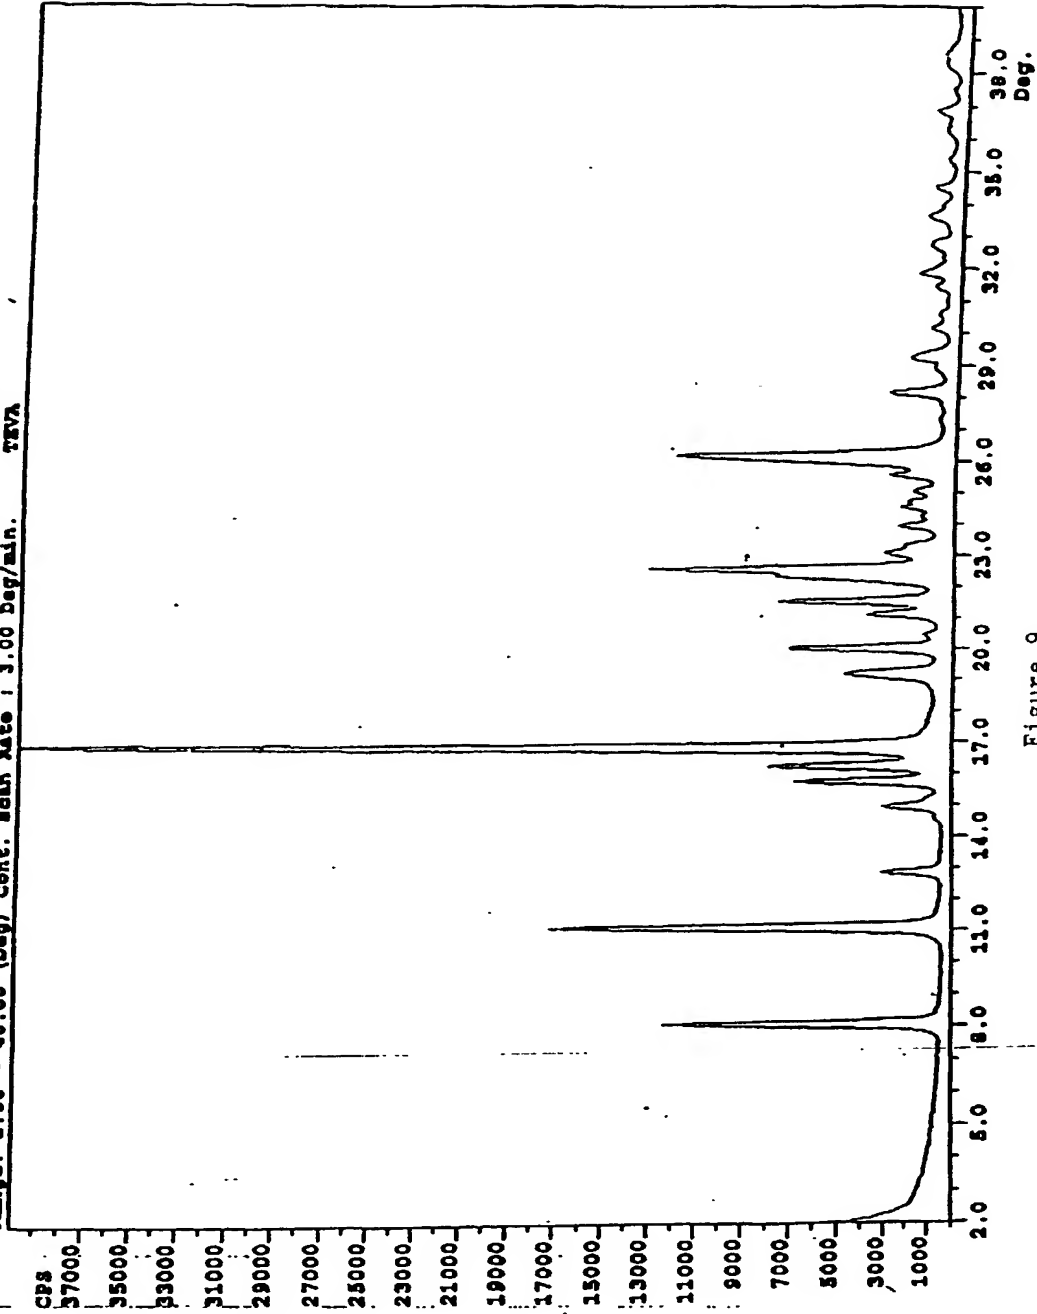


Figure 9

